

# Goat anti-Rat IgG (H+L) Cross-Adsorbed Secondary Antibody, Alexa Fluor™ 633

Product Details	
Size	1 mg
Species Reactivity	Rat
Host/Isotype	Goat / IgG
Class	Polyclonal
Type	Secondary Antibody
Conjugate	Alexa Fluor™ 633
Excitation/Emission Max	631/650 nm
Immunogen	Gamma Immunoglobins Heavy and Light chains
Form	Liquid
Concentration	2 mg/mL
Purification	purified
Storage buffer	PBS, pH 7.5
Contains	5mM sodium azide
Storage conditions	4° C, store in dark
RRID	AB_2535749


Applications	Tested Dilution	Publications
Western Blot (WB)	1:5,000-1:10,000	-
Immunohistochemistry (IHC)	-	0 Publication
Immunohistochemistry (Paraffin) (IHC (P))	1-10 µg/mL	0 Publication
Immunohistochemistry - Free Floating (IHC (Free))	-	0 Publication
Immunocytochemistry (ICC/IF)	1-2 µg/mL	0 Publication
Flow Cytometry (Flow)	-	0 Publication
Miscellaneous PubMed (Misc)	-	0 Publication

## Product Specific Information

Product will be shipped at Room Temperature.


**Rat IgG (H+L) Cross-Adsorbed Secondary Antibody (A-21094) in ICC/IF**

Immunofluorescence analysis of Goat anti-Rat IgG (H+L) Cross-Adsorbed Secondary Antibody, Alexa Fluor™ 633 (Product # A-21094) was performed using NTERA-2 (positive model) and HeLa (negative model) in cells stained with SOX2 Monoclonal Antibody (Btjce), eBioscience (Product # 14-9811-82). The cells were fixed with 4% paraformaldehyde for 10 minutes, permeabilized with 0.1% Triton™ X-100 for 10 minutes, blocked with 2% BSA for 1 hour and labeled with 1:100 dilution of primary antibody overnight at 4C. Goat anti-Rat IgG (H+L) Cross-Adsorbed Secondary Antibody, Alexa Fluor™ 633 (Product # A-21094, 1: 2000 dilution) in 0.1% BSA in PBS for 1 hour at room temperature, was used for detection of SOX2 in the nucleus (Panel a: Red). Nuclei (Panel b: blue) were stained with Hoechst33342 (Product # H1399). F-actin was stained with Alexa Fluor® 488 Phalloidin (Product # A12379, 1:500) (Panel c: green). Panel d represents the composite image. The specificity of the secondary antibody was proved by the absence of signal in HeLa (negative model for SOX2) due to no primary antibody binding (Panel e). Non-specific staining was not observed with secondary antibody alone (panel f). The images were captured at 40X magnification in CellInsight CX7 LZR High-Content Screening (HCS) Platform (Product # CX7A1110LZR) and externally deconvoluted (D.Sage et al./Methods 115 (2017) 28–41).

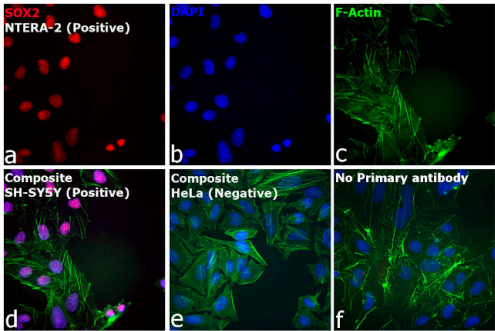


**Rat IgG (H+L) Cross-Adsorbed Secondary Antibody (A-21094) in ICC/IF**

Immunofluorescence analysis of Goat anti-Rat IgG (H+L) Secondary Antibody, Alexa Fluor® 633 was performed using A549 cells stained with alpha Tubulin (YL1/2) Rat Monoclonal Antibody (Product # MA1-80017). The cells were fixed with 4% paraformaldehyde for 10 minutes, permeabilized with 0.1% Triton™ X-100 for 10 minutes, blocked with 1% BSA for 1 hour and labeled with 2µg/mL Rat primary antibody for 3 hours at room temperature. Goat anti-Rat IgG (H+L) Secondary Antibody, Alexa Fluor® 633 (Product # A-21094) was used at a concentration of 2µg/mL in phosphate buffered saline containing 0.2% BSA for 45 minutes at room temperature, for detection of alpha Tubulin in the cytoplasm (Panel a: red). Nuclei (Panel b: blue) were stained with DAPI in SlowFade® Gold Antifade Mountant (Product # S36938). F-actin was stained with Alexa Fluor® 488 Phalloidin (Product # A12379, 1:300) (Panel c: green). Panel d represents the composite image. No nonspecific staining was observed with the secondary antibody alone (panel f), or with an isotype control (panel e). The images were captured at 60X magnification.

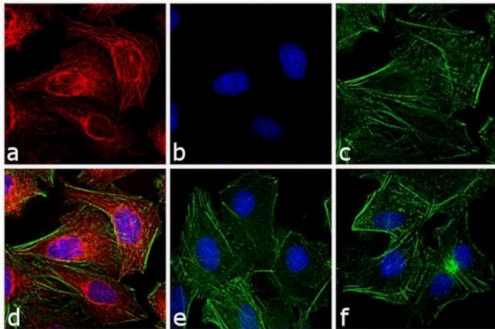

**Rat IgG (H+L) Cross-Adsorbed Secondary Antibody (A-21094) in IHC (P)**

Immunohistochemical analysis was performed on formalin-fixed paraffin-embedded mouse duodenum tissue section stained with Tubulin Rat Monoclonal Antibody (Product # MA1-80017) at 10 µg/mL in 0.1% normal goat serum overnight at 4 degree Celsius detected with Goat anti-Rat IgG (H+L) Cross-Adsorbed Secondary Antibody, Alexa Fluor™ 633 (Product # A-21094). Heat-induced epitope retrieval was performed on de-paraffinized sections using eBioscience™ IHC Antigen Retrieval Solution - Low pH (10X) (Product # 00-4955-58) in a decloaking chamber at 110 degrees Celsius for 15 minutes, followed by blocking with 2% normal goat serum, and then probing with primary and secondary antibodies. ReadyProbes™ Tissue Autofluorescence Quenching Kit (Product # R37630) was used to quench autofluorescence from the tissues. Nuclei were stained with DAPI (Product # D1306) and the sections were mounted using ProLong™ Glass Antifade Mountant (Product # P36984). The images were captured on EVOS™ M7000 Imaging System (Product # AMF7000) at 20X magnification and externally deconvoluted.

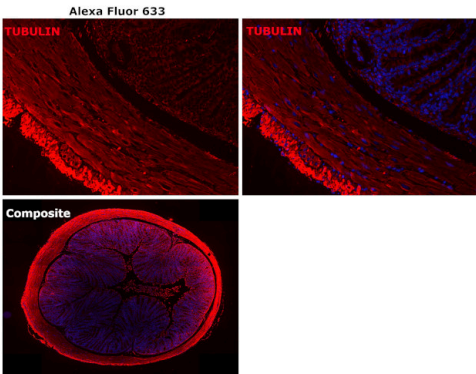

View more figures on [thermofisher.cn](https://thermofisher.cn)

Canonical and non-canonical PRC1 differentially contribute to regulation of neural stem cell fate. Life Sci Alliance (2025)

Loss of PRICKLE1 leads to abnormal endometrial epithelial architecture, decreased embryo implantation, and reduced fertility in mice. PNAS Nexus (2025)

Neonatal infection with Bordetella pertussis promotes autism-like phenotypes in mice. iScience (2025)

Dual-targeting CRISPR-CasRx reduces C9orf72 ALS/FTD sense and antisense repeat RNAs in vitro and in vivo. Nat Commun (2025)

Prefrontal gamma oscillations and fear extinction learning require early postnatal interneuron-oligodendroglia communication bioRxiv (2024)

For Research Use Only. Not for use in diagnostic procedures. Not for resale without express authorization. Products are warranted to operate or perform substantially in conformance with published Product specifications in effect at the time of sale, as set forth in the Production documentation, specifications and/or accompanying package inserts ("Documentation"). No claim of suitability for use in applications regulated by FDA is made. The warranty provided herein is valid only when used by properly trained individuals. Unless otherwise stated in the Documentation, this warranty is limited to one year from date of shipment when the Product is subjected to normal, proper and intended usage. This warranty does not extend to anyone other than the Buyer. Any model or sample furnished to Buyer is merely illustrative of the general type and quality of goods and does not represent that any Product will conform to such model or sample. NO OTHER WARRANTIES, EXPRESS OR IMPLIED, ARE GRANTED INCLUDING WITHOUT LIMITATION, IMPLIED WARRANTIES OF MERCHANTABILITY, FITNESS FOR ANY PARTICULAR PURPOSE, OR NON-INFRINGEMENT. BUYER'S EXCLUSIVE REMEDY FOR NON-CONFORMING PRODUCTS DURING THE WARRANTY PERIOD IS LIMITED TO REPAIR, REPLACEMENT OF OR REFUND FOR THE NON-CONFORMING PRODUCT(S) AT SELLER'S SOLE OPTION. THERE IS NO OBLIGATION TO REPAIR, REPLACE OR REFUND FOR PRODUCTS AS THE RESULT OF (I) ACCIDENT, DISASTER OR EVENT OF FORCE MAJEURE, (II) MISUSE, FAULT OR NEGLIGENCE OF OR BY BUYER, (III) USE OF THE PRODUCTS IN A MANNER FOR WHICH THEY WERE NOT DESIGNED, OR (IV) IMPROPER STORAGE AND HANDLING OF THE PRODUCTS. Unless otherwise expressly stated on the Product or in the documentation accompanying the Product, the Product is intended for research only and is not to be used for any other purpose, including without limitation, unauthorized commercial uses, in vitro diagnostic uses, ex vivo or in vivo therapeutic uses, or any type of consumption by or application to human or animals.