

Goat anti-Mouse IgG (H+L) Highly Cross-Adsorbed Secondary Antibody, Alexa Fluor™ Plus 488

Product Details	
Size	1 mg
Species Reactivity	Mouse
Host/Isotype	Goat / IgG
Class	Polyclonal
Type	Secondary Antibody
Conjugate	Alexa Fluor™ Plus 488
Excitation/Emission Max	493/518 nm
Immunogen	Gamma Immunoglobins Heavy and Light chains
Form	Liquid
Concentration	2 mg/mL
Purification	Affinity chromatography
Storage buffer	proprietary buffer, pH 6.5
Contains	0.016% Methylisothiazolone, 0.016% Bromonitrodioxane
Storage conditions	4° C, store in dark
RRID	AB_2633275

Applications	Tested Dilution	Publications
Western Blot (WB)	0.1-0.4 µg/mL	0 Publication
Immunohistochemistry (IHC)	-	0 Publication
Immunohistochemistry (Paraffin) (IHC (P))	-	0 Publication
Immunohistochemistry (PFA fixed) (IHC (PFA))	-	0 Publication
Immunohistochemistry (Frozen) (IHC (F))	-	0 Publication
Immunocytochemistry (ICC/IF)	1-10 µg/mL	0 Publication
Flow Cytometry (Flow)	-	0 Publication
Miscellaneous PubMed (Misc)	-	0 Publication

Product Specific Information

To minimize cross-reactivity, the goat anti-mouse IgG whole antibodies have been pre cross-adsorbed against bovine IgG, goat IgG, rabbit IgG, rat IgG, human IgG, and human serum. Cross-adsorption or pre-adsorption is a purification step to increase specificity of the antibody resulting in less background staining and cross-reactivity. The secondary antibody solution is passed through a column matrix containing immobilized serum proteins from potentially cross-reactive species. Only the nonspecific-binding secondary antibodies are captured in the column, and the highly specific secondaries flow through. Further passages through additional columns result in highly cross-adsorbed preparations of secondary antibody. The benefits of these extra steps are apparent in multiplexing/multicolor-staining experiments where there is potential cross-reactivity with other primary antibodies or in tissue/cell fluorescent staining experiments where there may be the presence of endogenous immunoglobulins.


Using conjugate solutions: Centrifuge the protein conjugate solution briefly in a microcentrifuge before use; add only the supernatant to the experiment. This step will help eliminate any protein aggregates that may have formed during storage,

thereby reducing nonspecific background staining. Because staining protocols vary with application, the appropriate dilution of antibody should be determined empirically.

Product Images For Goat anti-Mouse IgG (H+L) Highly Cross-Adsorbed Secondary Antibody, Alexa Fluor™ Plus 488


Mouse IgG (H+L) Highly Cross-Adsorbed Secondary Antibody (A32723) in ICC/IF

Immunofluorescence analysis of Goat anti-Mouse IgG (H+L) Highly Cross-Adsorbed Secondary Antibody, Alexa Fluor™ Plus 488 (Product # A32723) was performed using MCF 10A (positive model) and T-47D (negative model) cells stained with Vimentin Monoclonal Antibody (V9), eBioscience™ (Product # 14-9897-82). The cells were fixed with 4% paraformaldehyde for 10 minutes, permeabilized with 0.1% Triton™ X-100 for 10 minutes, blocked with 1% BSA for 1 hour and labeled with 2 µg/mL primary antibody for 3 hours at room temperature. Goat anti-Mouse IgG (H+L) Highly Cross-Adsorbed Secondary Antibody, Alexa Fluor™ Plus 488 (Product # A32723, 1:2000 dilution) in 0.1% BSA in PBS for 45 minutes at room temperature, was used for detection of Vimentin in the cytoskeleton (Panel a: Green). Nuclei (Panel b: blue) were stained with Hoechst33342 (Product # H1399). F-actin was stained with Alexa Fluor™ 647 Phalloidin (Product # A22287, 1:4000) (Panel c: red). Panel d represents the composite image. The specificity of the secondary antibody was proved by the absence of signal in T-47D (negative model for Vimentin) due to no primary antibody binding (Panel e). Non-specific staining was not observed with secondary antibody alone (panel f). The images were captured at 40X magnification in CellInsight CX7 LZR High-Content Screening (HCS) Platform (Product # CX7A1110LZR) and externally deconvoluted (D.Sage et al./Methods 115 (2017) 28–41).

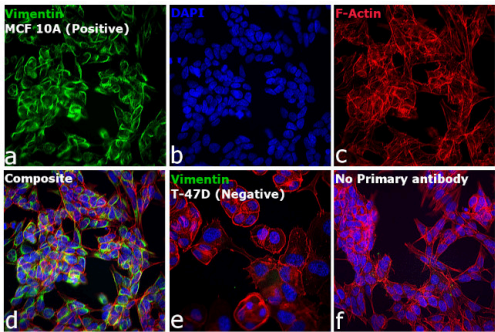


Mouse IgG (H+L) Highly Cross-Adsorbed Secondary Antibody (A32723) in ICC/IF

Immunofluorescence analysis of A32734, A-11081 and A32723 was performed using primary antibodies against Pericentrin (Product # PA5-53498), alpha Tubulin (Product # MA1-80017) and ATP5A1 (Product # 43-9800) in 70% confluent log phase HEK 293 cells. The cells were fixed with 4% Paraformaldehyde, permeabilized with 0.1% Triton X-100 and blocked with 2% BSA, then incubated with the primary antibodies at 1:100 dilution each at 4 degree celsius overnight. The cells were then incubated with Goat anti-Rabbit IgG (H+L) Highly Cross-Adsorbed Secondary Antibody, Alexa Fluor Plus 680 (Product # A32734), Goat anti-Rat IgG (H+L) Cross-Adsorbed Secondary Antibody, Alexa Fluor 546 (Product # A-11081) and Goat anti-Mouse IgG (H+L) Highly Cross-Adsorbed Secondary Antibody, Alexa Fluor Plus 488 (Product # A32723) at 1:2000 dilution each in 0.1% BSA at room temperature for 45 minutes. The images were captured at 40X magnification in CellInsight CX7 LZR High-Content Screening (HCS) Platform (Product # CX7A1110LZR) and externally deconvoluted (D.Sage et al./Methods 115 (2017) 28–41). The specific centrosomal, cytoskeletal and mitochondrial localization of Pericentrin (Panel a), Tubulin (Panel b) and ATP5A1 (Panel c) in the respective channels alone shows the specificity of all the 3 secondary antibodies used. Nuclei (Panel d) were stained with Hoechst33342 (Product # H1399). Panel e is the composite of Panels a-d, showing co-localisation. Panel f is control cells with no primary antibody.

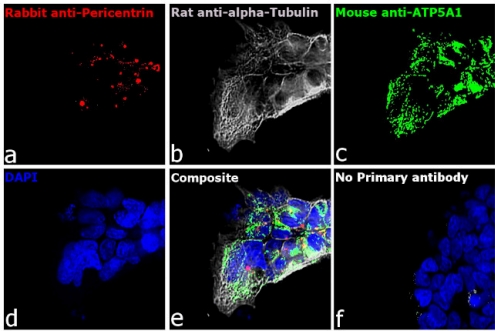

Mouse IgG (H+L) Highly Cross-Adsorbed Secondary Antibody (A32723) in ICC/IF

Immunofluorescence analysis of A-32723, A-11081 and A-32734 was performed using primary antibodies against Survivin (Product # 14-9176-82), alpha Tubulin (Product # MA1-80017) and KIF11 (Product # MA5-32792) in 70% confluent log phase Caco-2 cells. The cells were fixed with 4% Paraformaldehyde, permeabilized with 0.1% Triton X-100 and blocked with 2% BSA, then incubated with the primary antibodies at 1:100 dilution each at 4 degree celsius overnight. The cells were then incubated with Goat anti-Mouse IgG (H+L) Highly Cross-Adsorbed Secondary Antibody, Alexa Fluor™ Plus 488 (Product # A32723), Goat anti-Rat IgG (H+L) Cross-Adsorbed Secondary Antibody, Alexa Fluor™ 546 (Product # A-11081) and Goat anti-Rabbit IgG (H+L) Highly Cross-Adsorbed Secondary Antibody, Alexa Fluor™ Plus 680 (Product # A-32734) at 1:2000 dilution each in 0.1% BSA at room temperature for 45 minutes. The images were captured at 40X magnification in CellInsight CX7 LZR High-Content Screening (HCS) Platform (Product # CX7A1110LZR) and externally deconvoluted (D.Sage et al./Methods 115 (2017) 28–41). The specific translocation of each protein during each stage of mitosis is visible in the respective channel alone (Tubulin-green), (KIF11-Magenta) and Survivin-Red). This shows the specificity of all the 3 secondary antibodies used. Nuclei (Panel d) were stained with Hoeschst (Product # P36962). Panels e,j,o and t are merged images showing co-localisation.

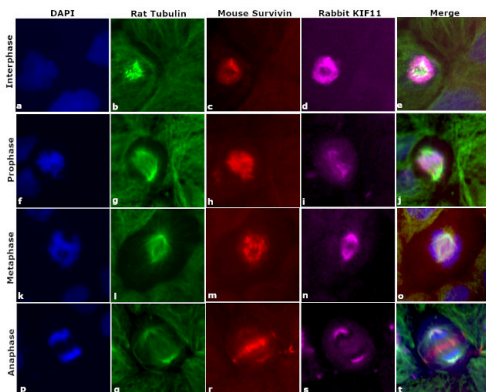

[View more figures on thermofisher.cn](https://thermofisher.cn)

1351 References

Engineering aortic valves via transdifferentiating fibroblasts into valvular endothelial cells without using viruses or iPS cells. *Bioact Mater* (2025)

Development of a Microphysiological System to Model Human Cancer Metastasis From the Colon to the Liver. *Biotechnol Bioeng* (2025)

A force-sensitive adhesion GPCR is required for equilibrioception. *Cell Res* (2025)

Accelerated epigenetic aging in Huntington's disease involves polycomb repressive complex 1. *Nat Commun* (2025)

A pumpless microfluidic co-culture system to model the effects of shear flow on biological barriers. *Lab Chip* (2025)

For Research Use Only. Not for use in diagnostic procedures. Not for resale without express authorization. Products are warranted to operate or perform substantially in conformance with published Product specifications in effect at the time of sale, as set forth in the Production documentation, specifications and/or accompanying package inserts ("Documentation"). No claim of suitability for use in applications regulated by FDA is made. The warranty provided herein is valid only when used by properly trained individuals. Unless otherwise stated in the Documentation, this warranty is limited to one year from date of shipment when the Product is subjected to normal, proper and intended usage. This warranty does not extend to anyone other than the Buyer. Any model or sample furnished to Buyer is merely illustrative of the general type and quality of goods and does not represent that any Product will conform to such model or sample. NO OTHER WARRANTIES, EXPRESS OR IMPLIED, ARE GRANTED INCLUDING WITHOUT LIMITATION, IMPLIED WARRANTIES OF MERCHANTABILITY, FITNESS FOR ANY PARTICULAR PURPOSE, OR NON-INFRINGEMENT. BUYER'S EXCLUSIVE REMEDY FOR NON-CONFORMING PRODUCTS DURING THE WARRANTY PERIOD IS LIMITED TO REPAIR, REPLACEMENT OF OR REFUND FOR THE NON-CONFORMING PRODUCT(S) AT SELLER'S SOLE OPTION. THERE IS NO OBLIGATION TO REPAIR, REPLACE OR REFUND FOR PRODUCTS AS THE RESULT OF (i) ACCIDENT, DISASTER OR EVENT OF FORCE MAJEURE, (ii) MISUSE, FAULT OR NEGLIGENCE OF OR BY BUYER, (iii) USE OF THE PRODUCTS IN A MANNER FOR WHICH THEY WERE NOT DESIGNED, OR (iv) IMPROPER STORAGE AND HANDLING OF THE PRODUCTS. Unless otherwise expressly stated on the Product or in the documentation accompanying the Product, the Product is intended for research only and is not to be used for any other purpose, including without limitation, unauthorized commercial uses, in vitro diagnostic uses, ex vivo or in vivo therapeutic uses, or any type of consumption by or application to human or animals.